


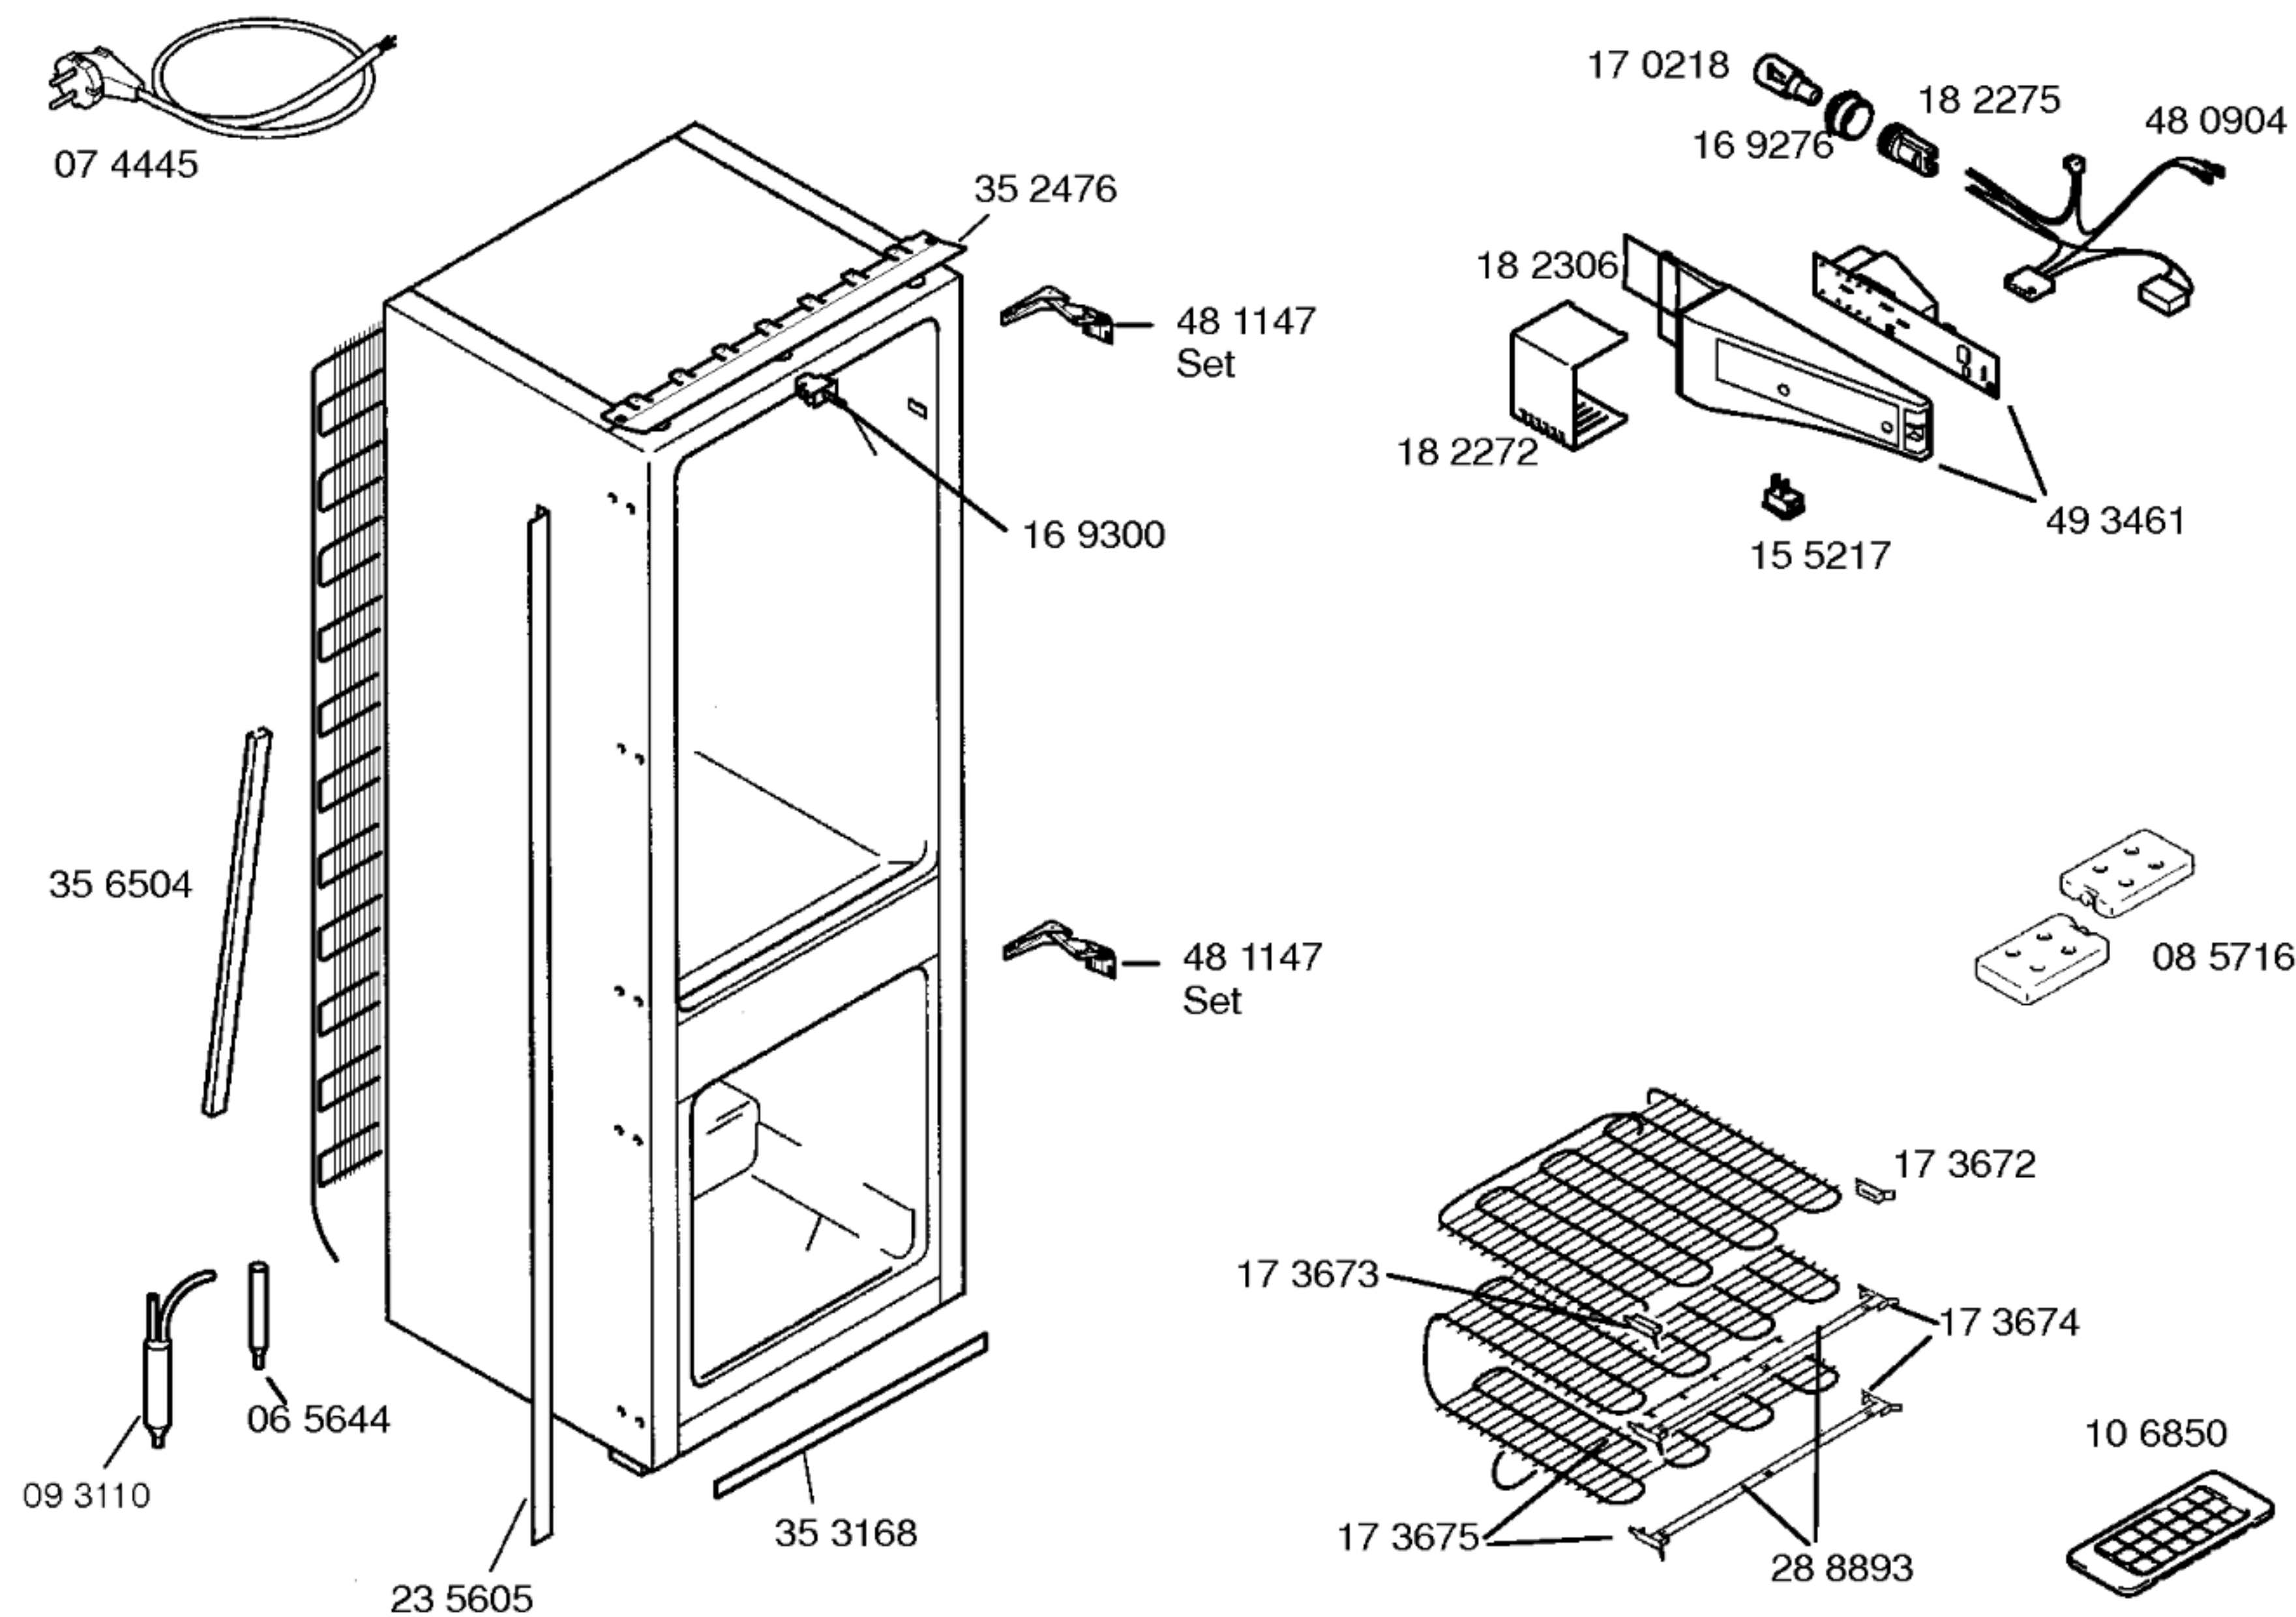
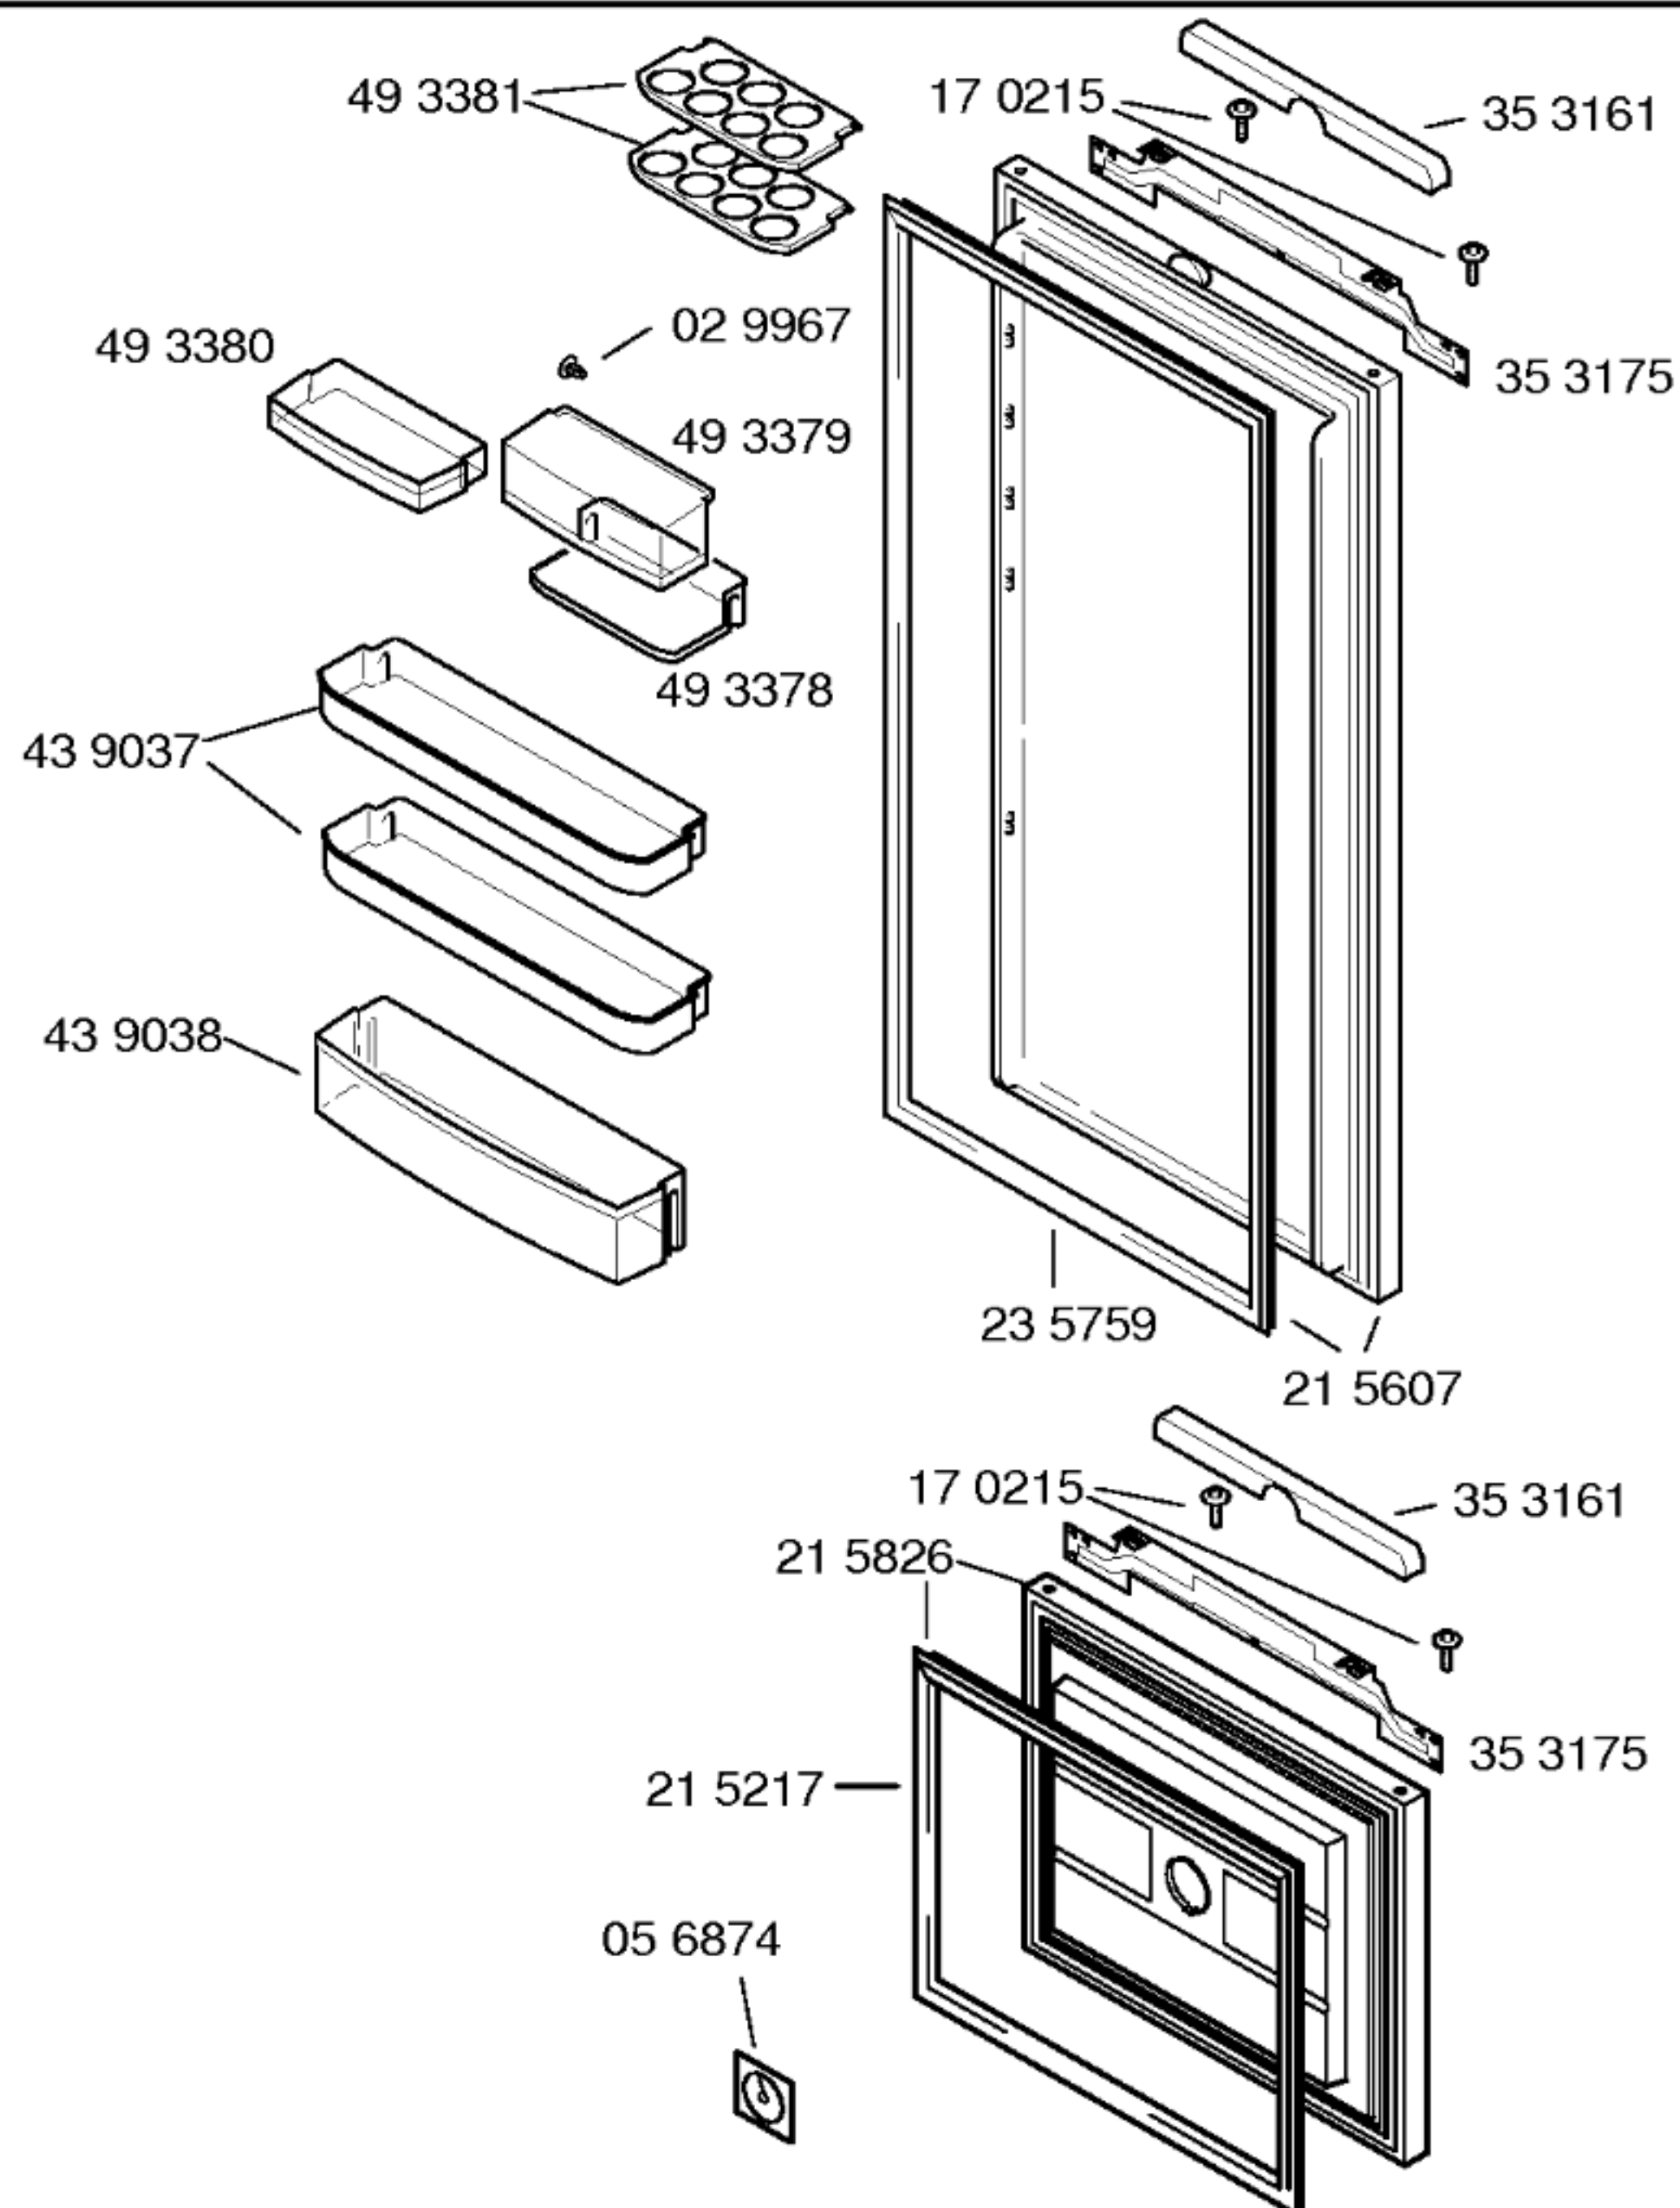
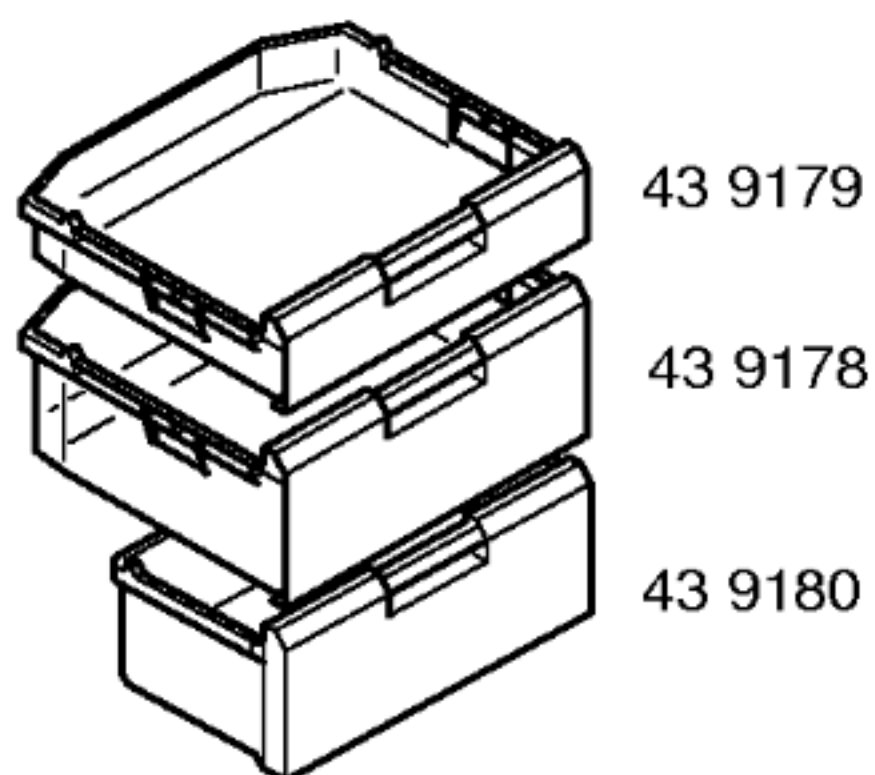


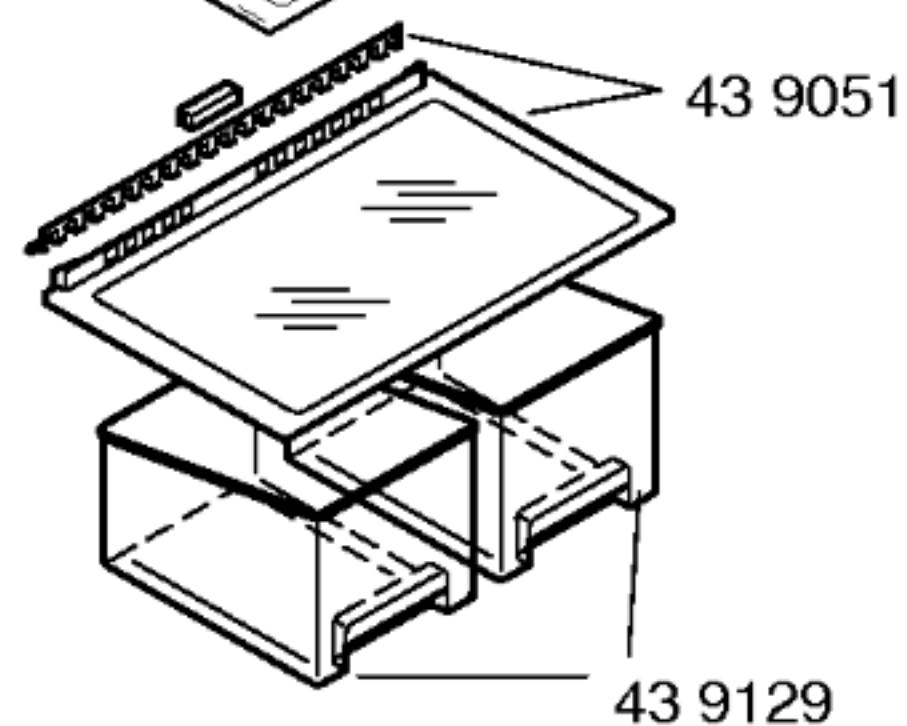

Mat. - Nr. - Konstante
3740

Gebrauchsanweisung
59 0393
(de,en)
Montageanleitung
58 8057
Befestigungssatz
26 6910

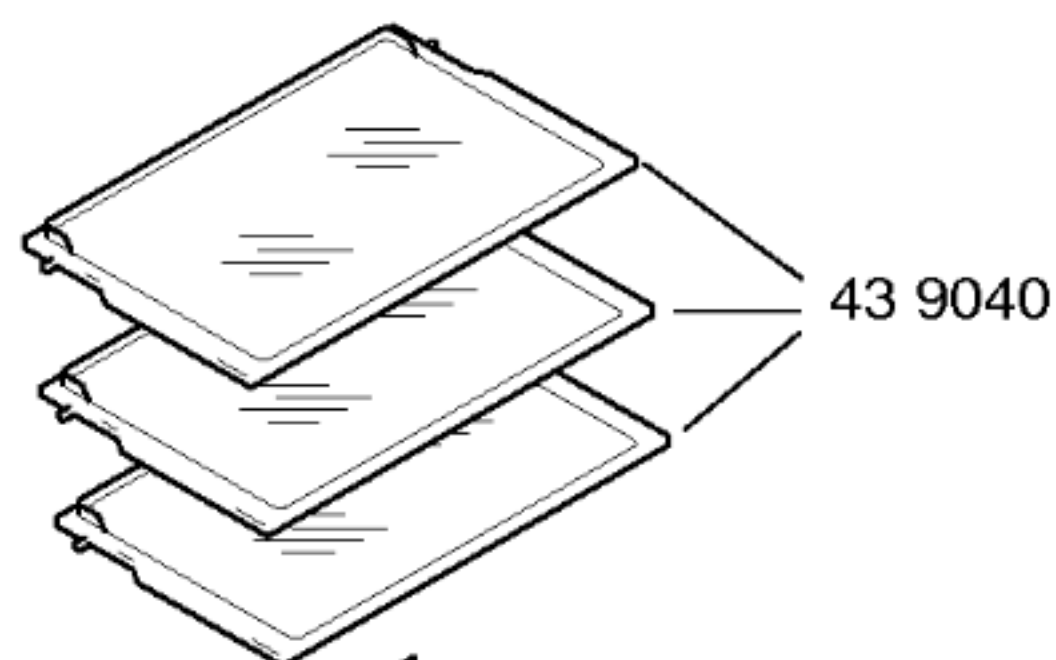

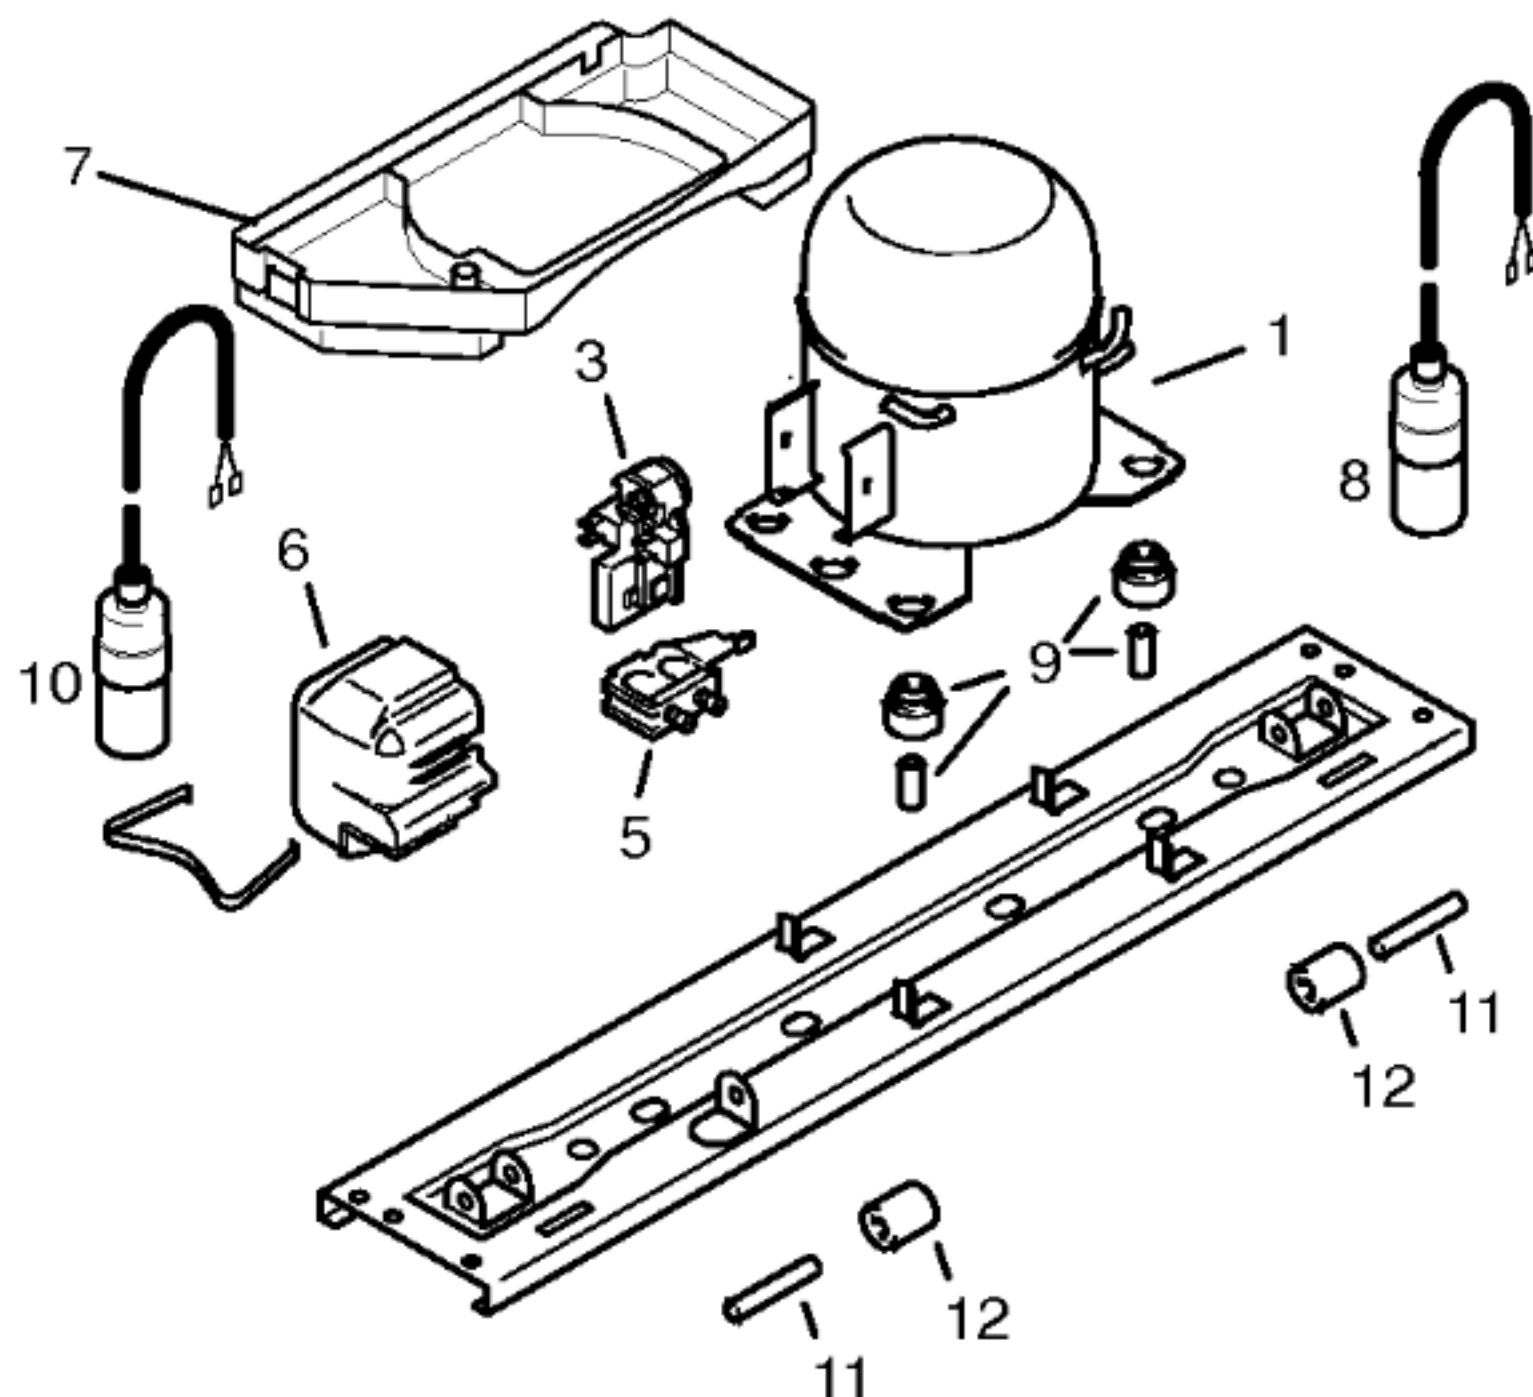

	V01-V02	V03,V04	
Pos.	Matsushita	Danfoss	
	DGX 110 E	NLX11KK2	
1	14 2360	14 4254	
2			
3	18 8959	42 6099	
4			
5	18 3590	15 0760	
6	41 8045	15 1072	
7	26 6624	441089	
8	41 9025		
9	05 0166	05 0166	
10	16 8603	15 2222	
11			
12			

TECHNISCHE DATEN / TECHNICAL DATA / DONNEES TECHNIQUES			
Verdichter/Compressor/Compresseur		Matsushita	Danfoss
Typ/Type		DGX 110 E	NLX11KK2
Förderleistung/Delivery/Débit	l/h	1955	2007
Anlaufstrom/Starting current/Cour de démarrage	A	0,5	7,8
Widerstand/Resistance/Résistance	W	14,7	16,5
	Hi/aux	W	27,3
Temp.-Regler/Thermostat			
Typ/Type			
Regelstellung/Position			
Schaltwerte/Switching values	"warm"		
Valeurs de commutation	"kalt"		
	"alarm"		
Füllmenge/Fill.quantity/Charge	R600a	*	
Anschlußwert/Conn.load/Puiss. connectée	W	104	130
Heizung/Heater/Chauffage			
Widerstand/Resistance/Résistance	W		
Leistung/Power/Puissance	W		
Ventilator/Blower/Ventilateur			
Widerstand/Resistance/Résistance	W		
Raumtemperaturfühler			
Widerstand NTC-Fühler			
Magnetventil/Magnetic valve/Electrovanne			
Widerstand/Resistance/Résistance	W		
Spannung/Voltage/Tension	V		

* siehe Typenschild